Dräger

MicroVent
SW 1.10

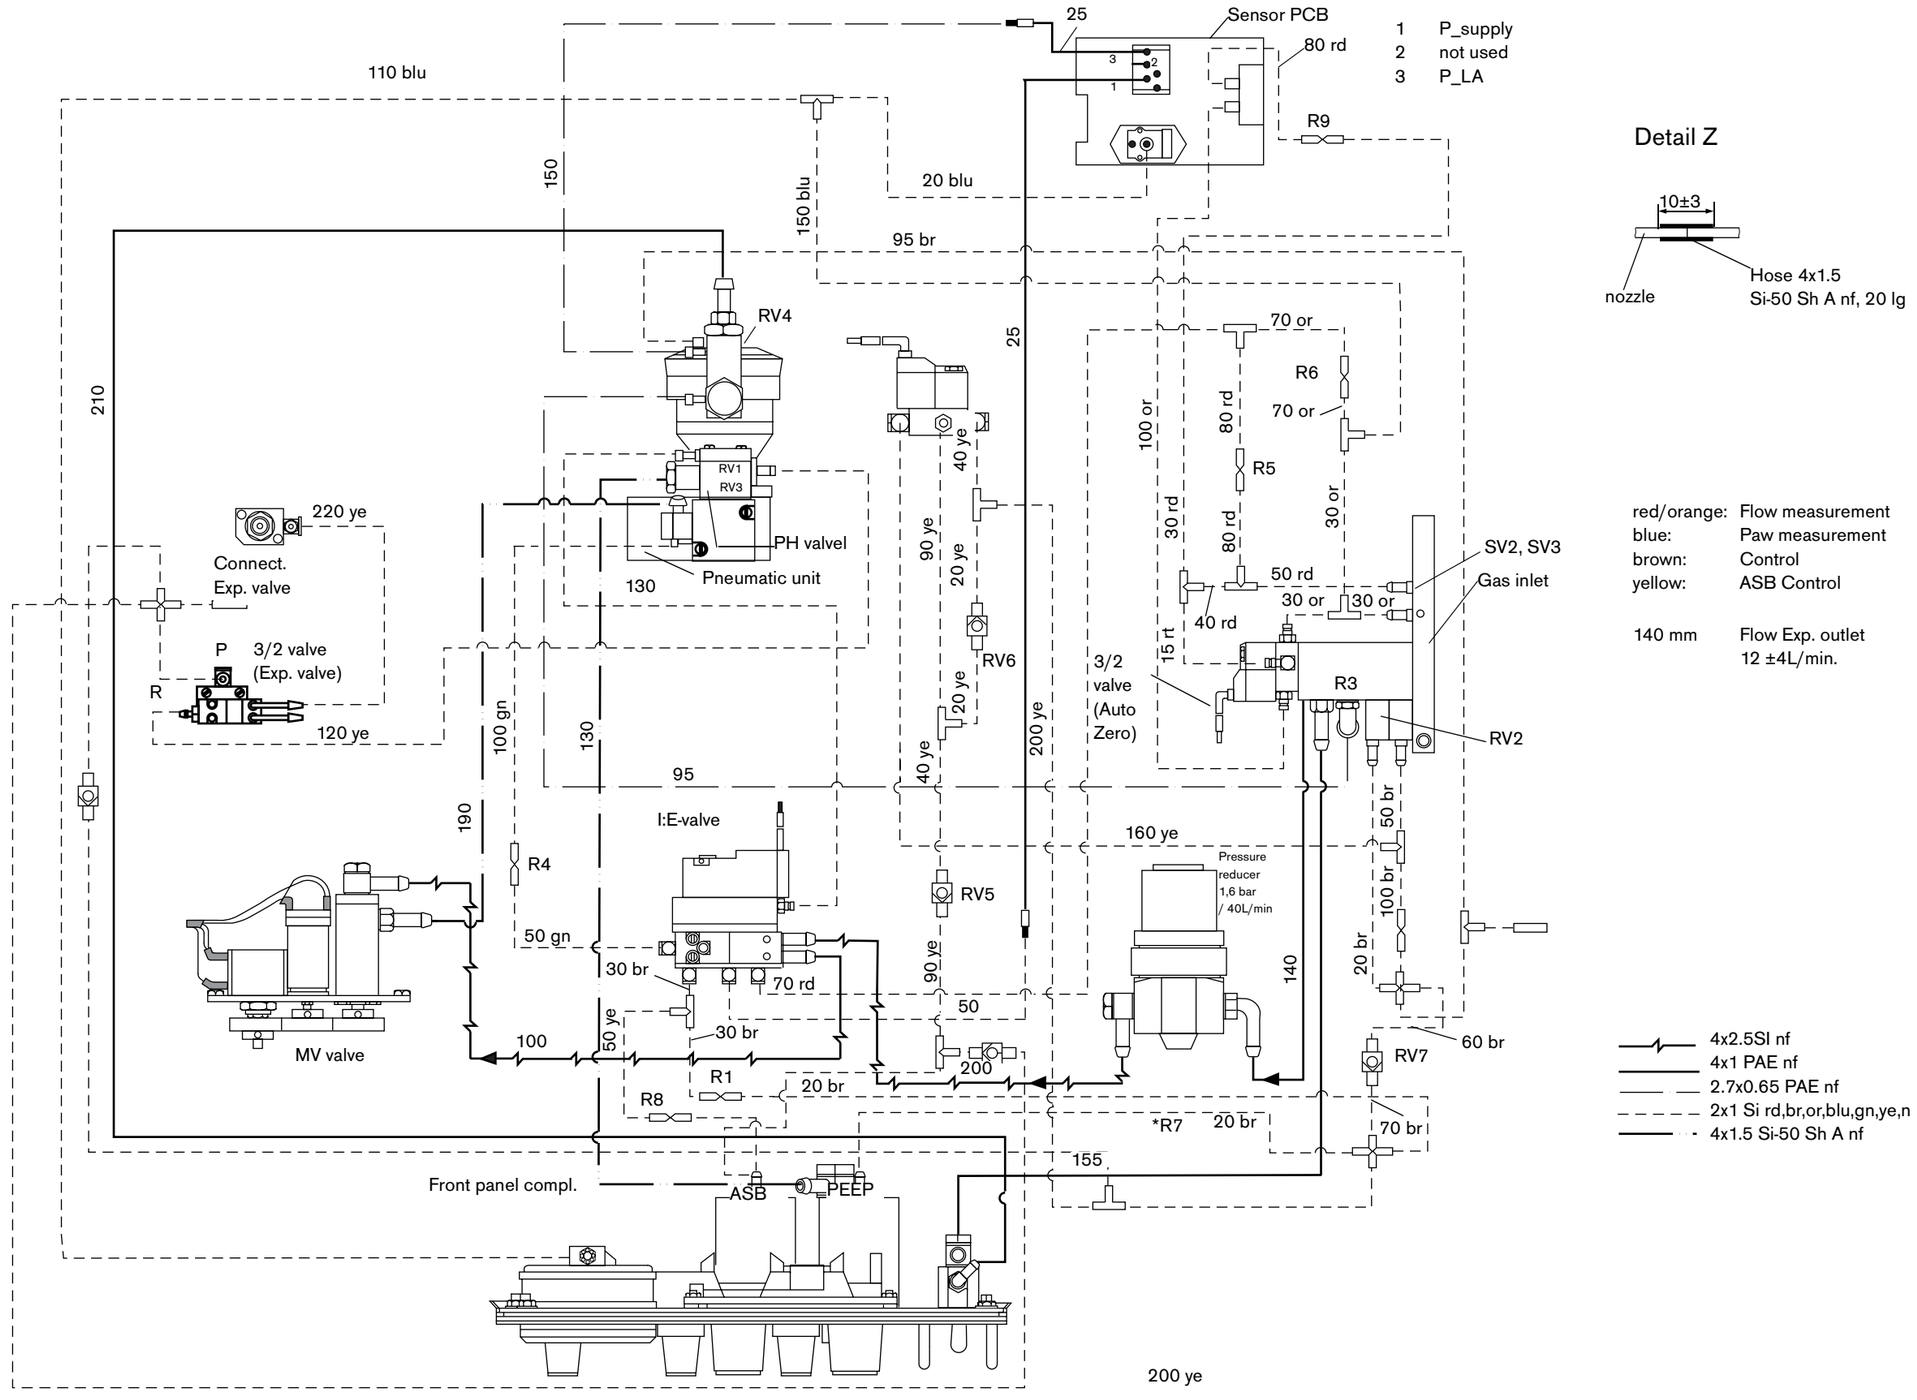

Detail Z

red/orange: Flow measurement
blue: Paw measurement
brown: Control
yellow: ASB Control

140 mm Flow Exp. outlet
12 ±4L/min.

4x2.5Sl nf
4x1 PAE nf
2.7x0.65 PAE nf
2x1 Si rd,br,or,blu,gn,ye,n
4x1.5 Si-50 Sh A nf

Hosediagrame.fm
For internal use only. Copyright reserved.

MicroVent
SW 1.21

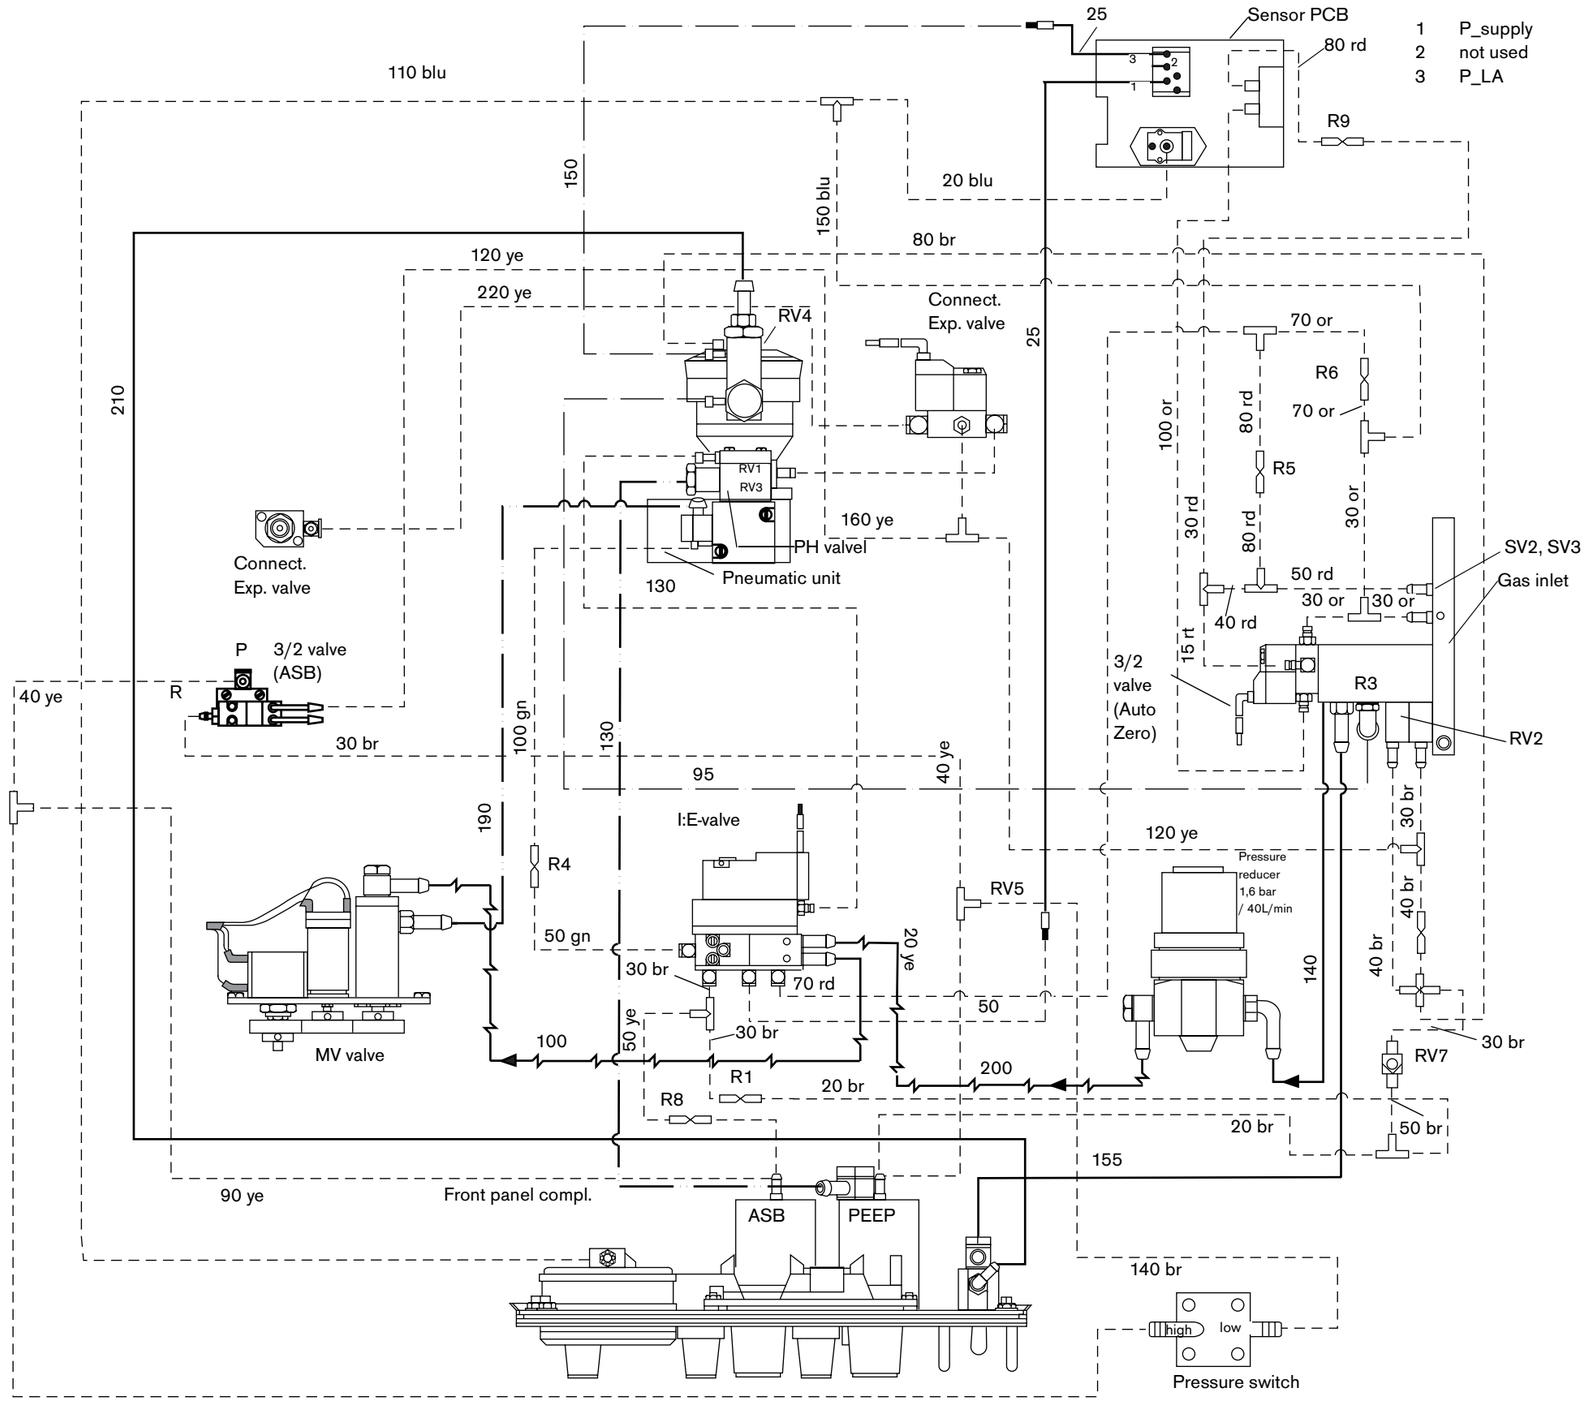

Detail Z

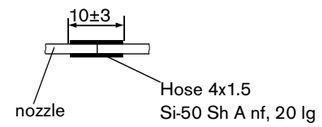

red/orange: Flow measurement
blue: Paw measurement
brown: Control
yellow: ASB Control

140 mm Flow Exp. outlet
12 ±4L/min.

4x2.5Sl nf
4x1 PAE nf
2.7x0.65 PAE nf
2x1 Si rd,br,or,blu,gn,ye,n
4x1.5 Si-50 Sh A nf

Hosediagram2e.fm
For internal use only. Copyright reserved.

MicroVent
SW 1.21

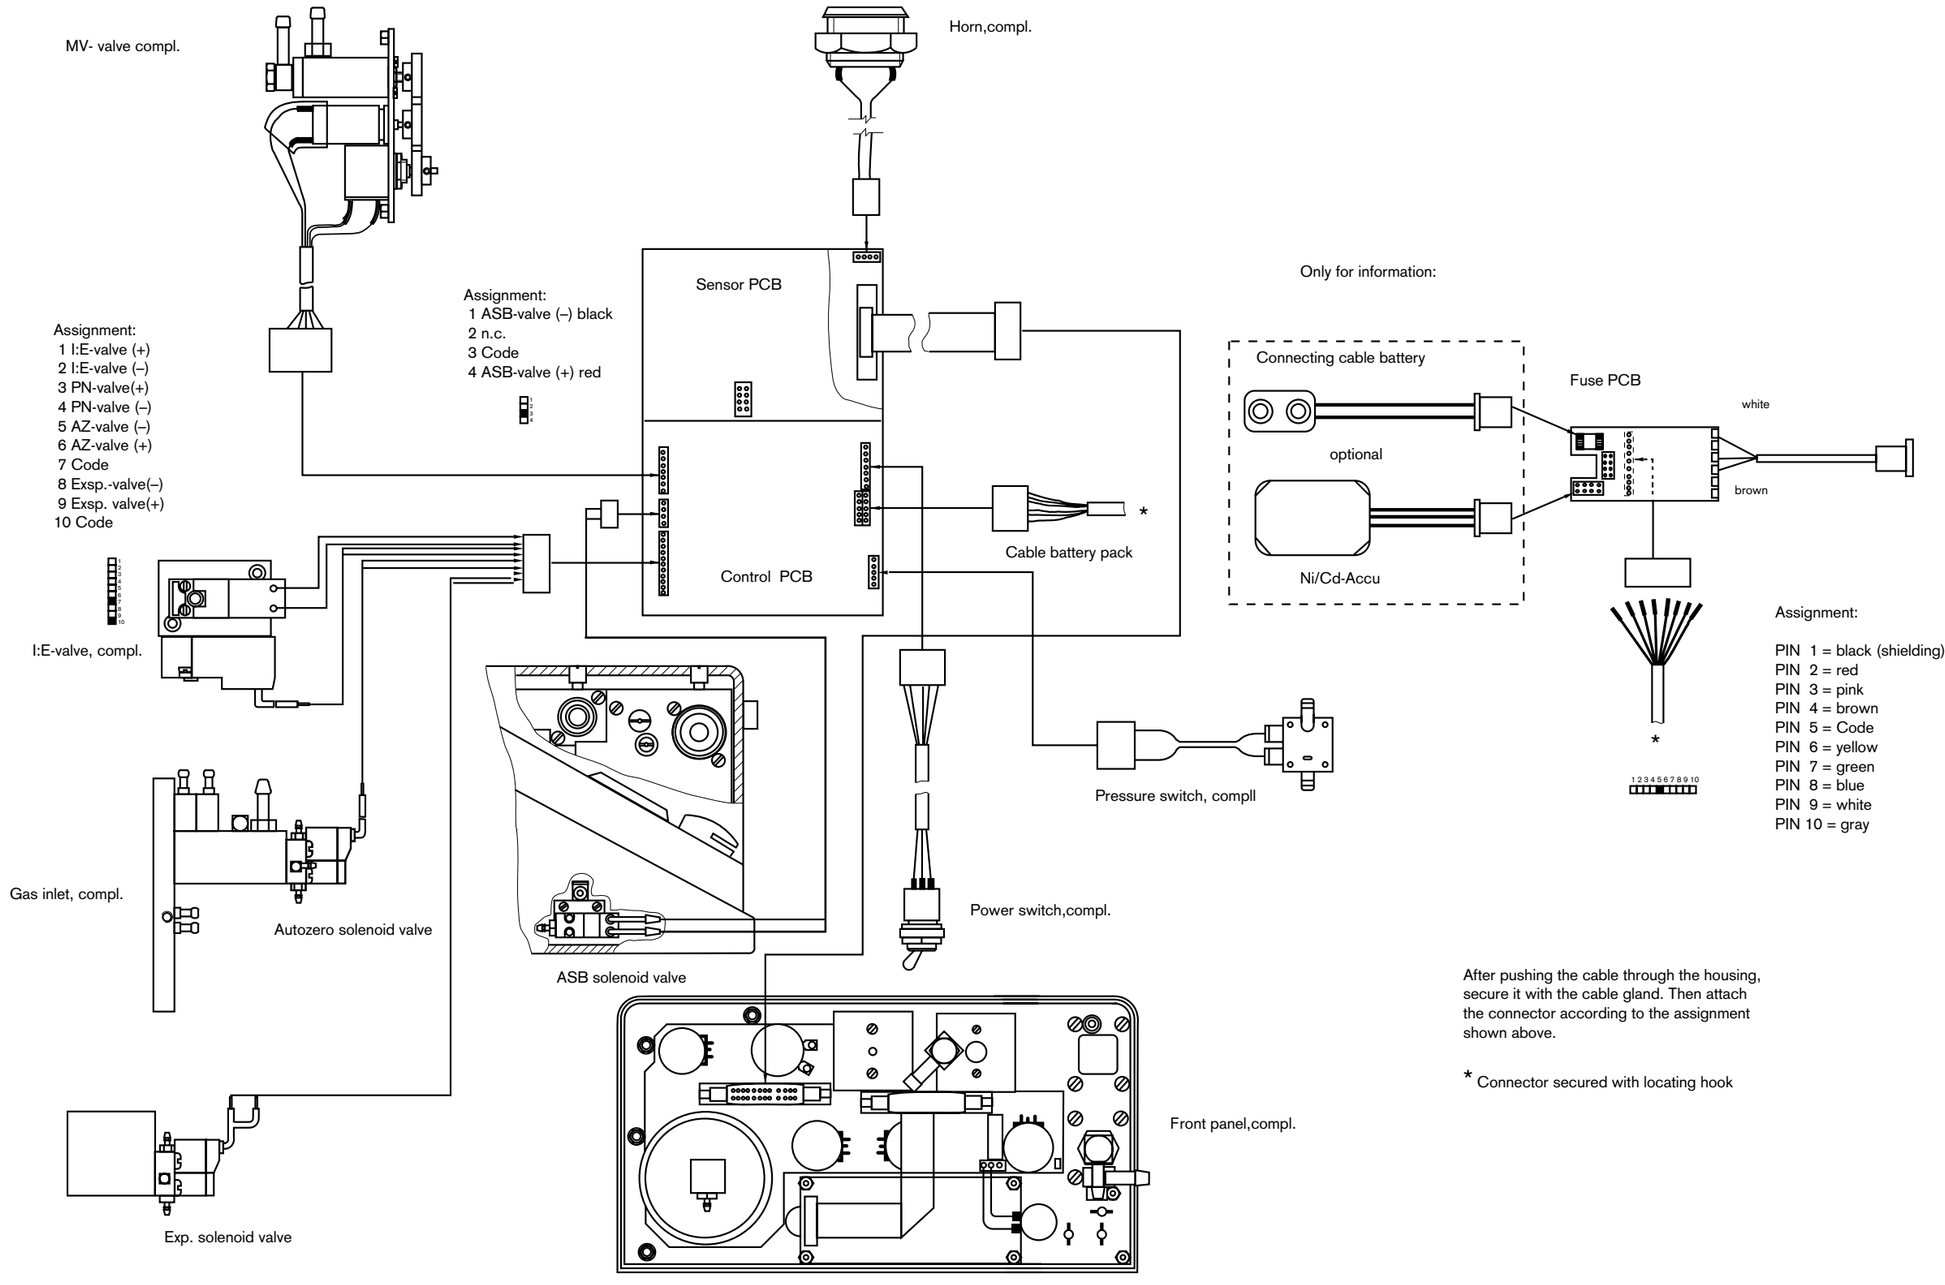

Only for information:

Assignment:

PIN 1 = black (shielding)
PIN 2 = red
PIN 3 = pink
PIN 4 = brown
PIN 5 = Code
PIN 6 = yellow
PIN 7 = green
PIN 8 = blue
PIN 9 = white
PIN 10 = gray

After pushing the cable through the housing, secure it with the cable gland. Then attach the connector according to the assignment shown above.

* Connector secured with locating hook

Interconnecting diagram (Micro Vent)

Anschlussplan2(Micro)eA3.fm
For internal use only. Copyright reserved.

MicroVent
SW 1.10

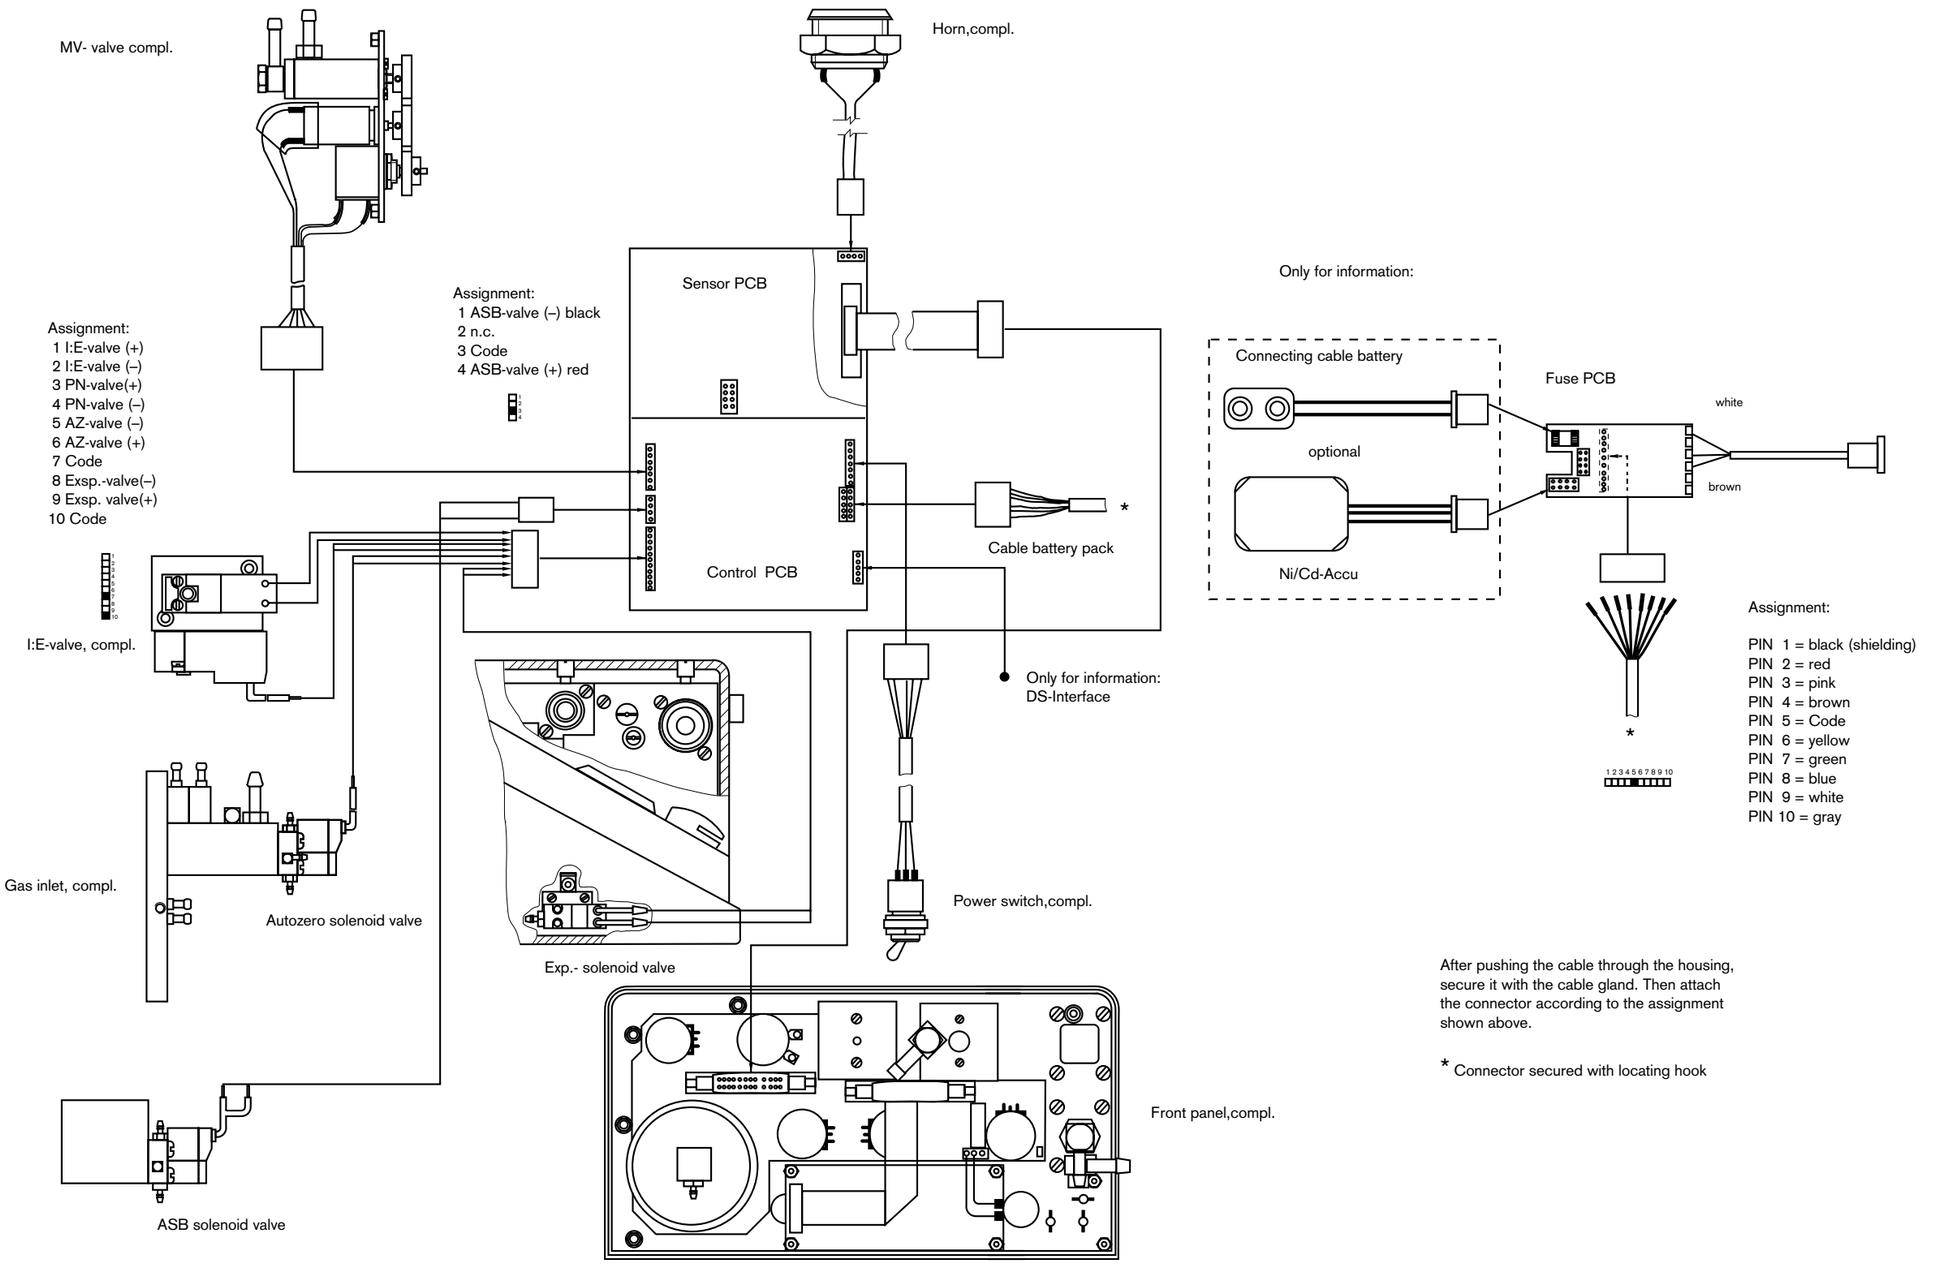

Only for information:

Assignment:

PIN 1 = black (shielding)
PIN 2 = red
PIN 3 = pink
PIN 4 = brown
PIN 5 = Code
PIN 6 = yellow
PIN 7 = green
PIN 8 = blue
PIN 9 = white
PIN 10 = gray

After pushing the cable through the housing, secure it with the cable gland. Then attach the connector according to the assignment shown above.

* Connector secured with locating hook

Interconnecting diagram (Micro Vent)

Anschlussplan(Micro)eA3.fm
For internal use only. Copyright reserved.